ASM

User Instructions

ASM Wren Kitchen / Shower Stool Range.




Picow Farm Road Ind Estate Runcorn. Cheshire. WA7 4UG. Tel: 01928 574301

Fax: 01928 575130 E-mail: sales@asmmedicare.com



Wren Kitchen / Shower Stool Range.



Codes: 02300 / 02301 / 02302 / 02303 & 02304

The ASM Wren Stools come fully assembled and ready for use. With the exception of 02300, the stools are height adjustable, with optional starting heights of 483mm (19") to 635mm (25") or 559mm (22") to 711mm (28").

To adjust please follow the instructions below.

1} Place the stool on it's side and remove the plastic clips from 2 legs. See Fig 1.

2} Slide the adjustable internal legs to the required position ensuring that both legs are adjusted equally. See Fig 1. The stools are **NOT** designed to be used with the seats level.

3} Replace the plastic clips, ensuring that they are **fully engaged**. You may have to twist the leg slightly to locate the steel pin correctly.

4} Turn the stool over & repeat for the other two adjustable legs.

5} Place the chair upright on it's feet on a level surface & check that it is stable and does not rock, if it does readjust the legs until it is stable.

6) Periodic checks of all screws and fittings is recommended, replace if required.

7} To clean the stool, a mild proprietary soap and / or disinfectant may be used.

After cleaning dry with a soft clean cloth.

The Maximum User Weight for this product is: 152kg / 24st.

The intended use of this product is to provide the user with a "perching" type seat for those unable to sit fully.

NOTE:- These products are only to be used for their intended purpose. For details of all our products please visit our web site at www.asmmedicare.com

Better By Design




IMPORTANT NOTICE!

Please read & fully understand before using or allowing others to do so.



April 2009.

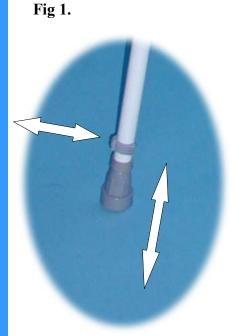

To avoid injury please DO NOT attempt to move these products whilst the patient / user is seated!